Nitrile Exam Gloves

REF PM6-270X

Accelerator Free | Chemo Drug Tested | Textured Fingertips | Powder-free | Indigo

ABOUT THE GLOVE

Glove users gravitate to latex-free alternatives, skin irritations to non-latex gloves are becoming more prevalent. Although much less severe than the potential of a latex allergy, these Type IV dermatitis sensitivities can cause issues for some people. The PRIMED Pure* nitrile gloves are manufactured without chemical accelerators that are found in most nitrile gloves which further protects you from material sensitivities.

Pure*

PROTECTION STANDARDS

Exceeds the current ASTM D6319: Standard Specification for Nitrile Examination Gloves for Medical Application.

Tested against chemotherapy drugs to the current ASTM D6978: Standard Practice for Assessment of Resistance of Medical Gloves to Permeation by Chemotherapy Drugs.
(Additional information available.)

Tested to ASTM F1671 for Viral Penetration.

FEATURES & BENEFITS

Lightweight Nitrile Technology

Combines strength with tactile sensitivity, allowing intricate and precise movement.

Flexible and Comfortable Fit


Moves with the wearer to facilitate natural dexterity.

Fully Micro-textured with Enhanced Fingertip Texturing

Provides reliable grip when handling small instruments and objects.

Low Derma — Accelerator Free Nitrile

Prevents Type IV allergies (Dermatitis) in users with sensitivities.

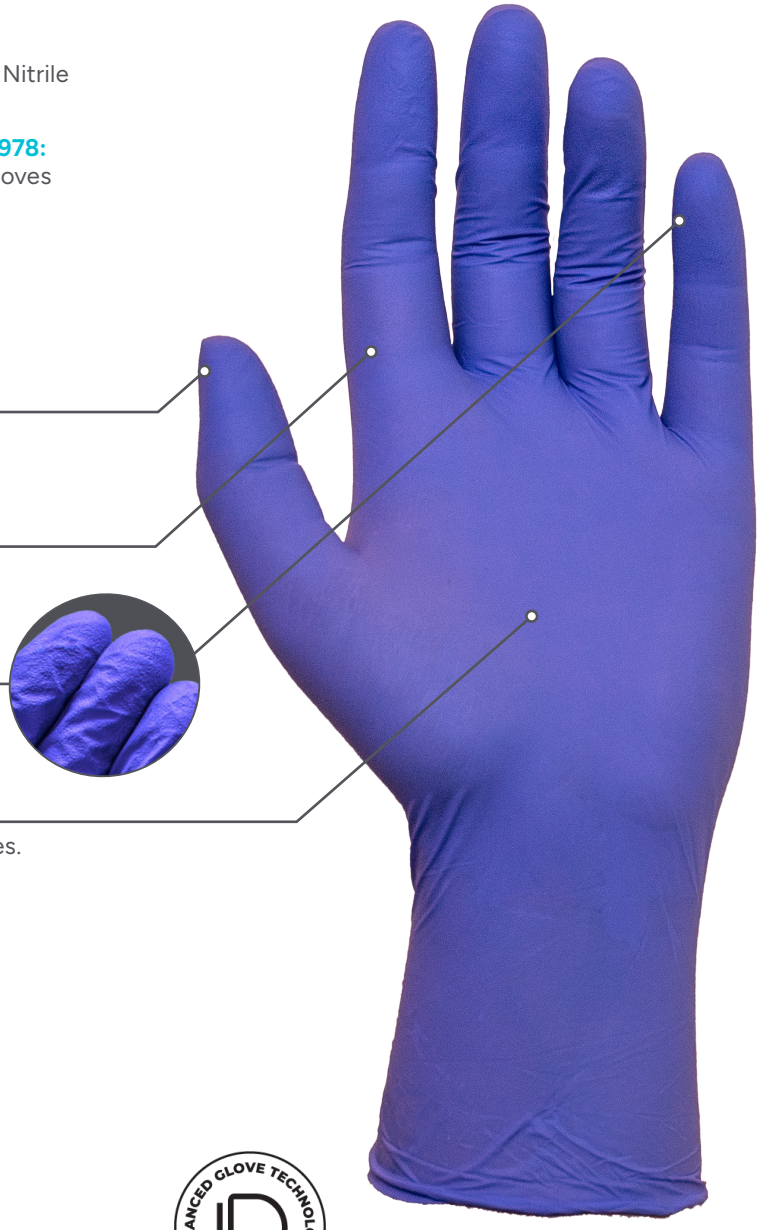

AVAILABLE SIZES

XS	S	M	L	XL
PM6-2705	PM6-2706	PM6-2707	PM6-2708	PM6-2709



QUANTITIES

GLOVES/BOX	BOXES/CASE	GLOVES/CASE
150	10	1500

ADVANCED GLOVE TECHNOLOGY · LOW DERMA™ ·

MD LATEX NON STERILE

PRI·MED MEDICAL PRODUCTS

PRIMED Medical Products Inc.
200, 2003-91 Street SW, Edmonton, AB, Canada, T6X 0W8
TF +1.877.877.4633 | F +1.780.497.7670 | W PRIMED.com | E info@PRIMED.com

*Registered Trademark or Trademark of PRIMED Medical Products Inc. or its affiliates.

NA-REVC1