

# Enbio PRO.
## Small footprint. Big space.

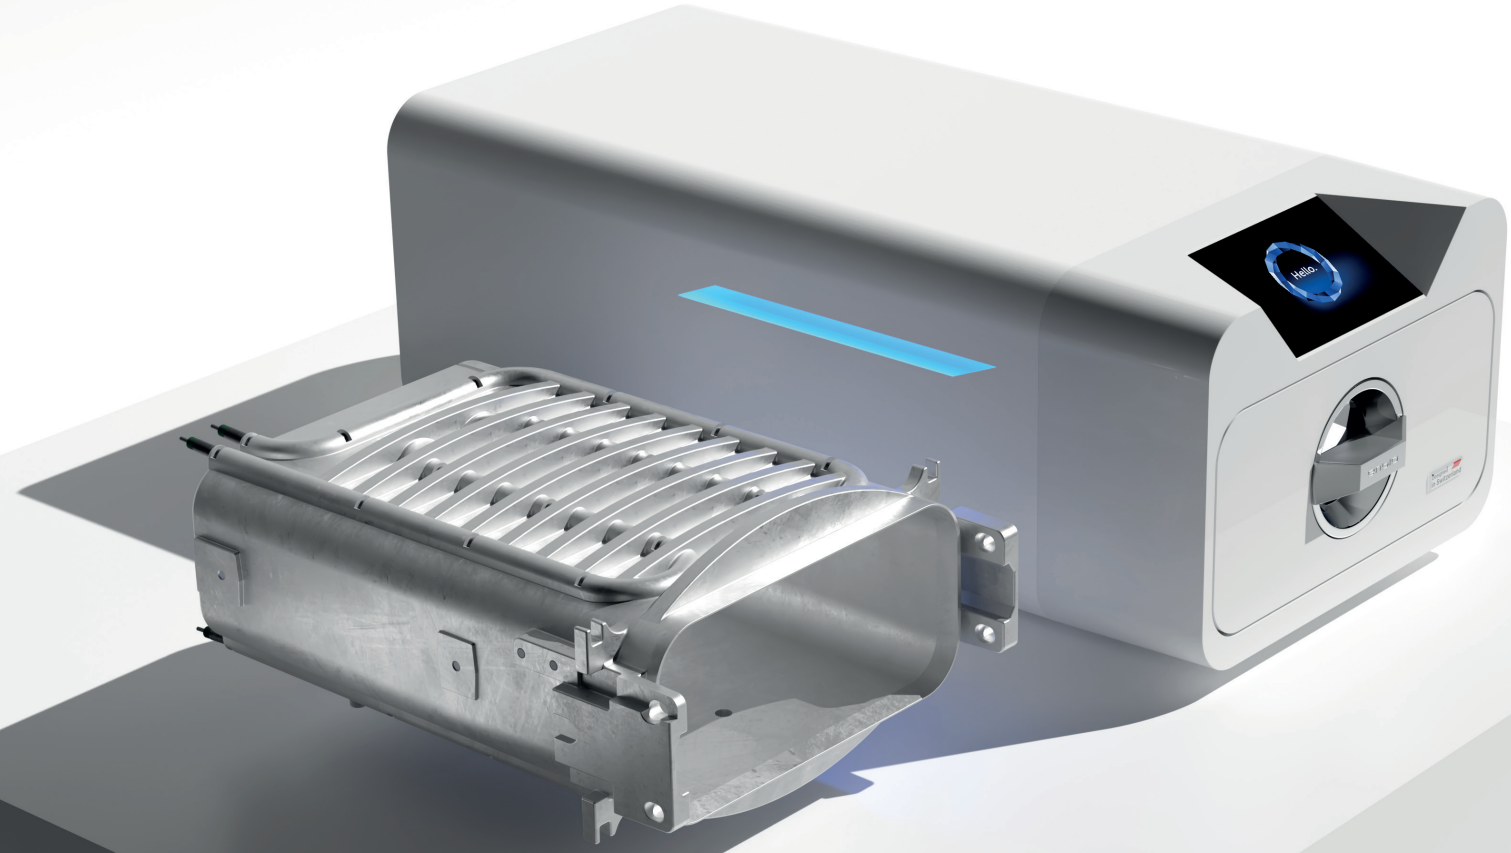

Triple Vacuum
Full Drying

Designed
in Switzerland

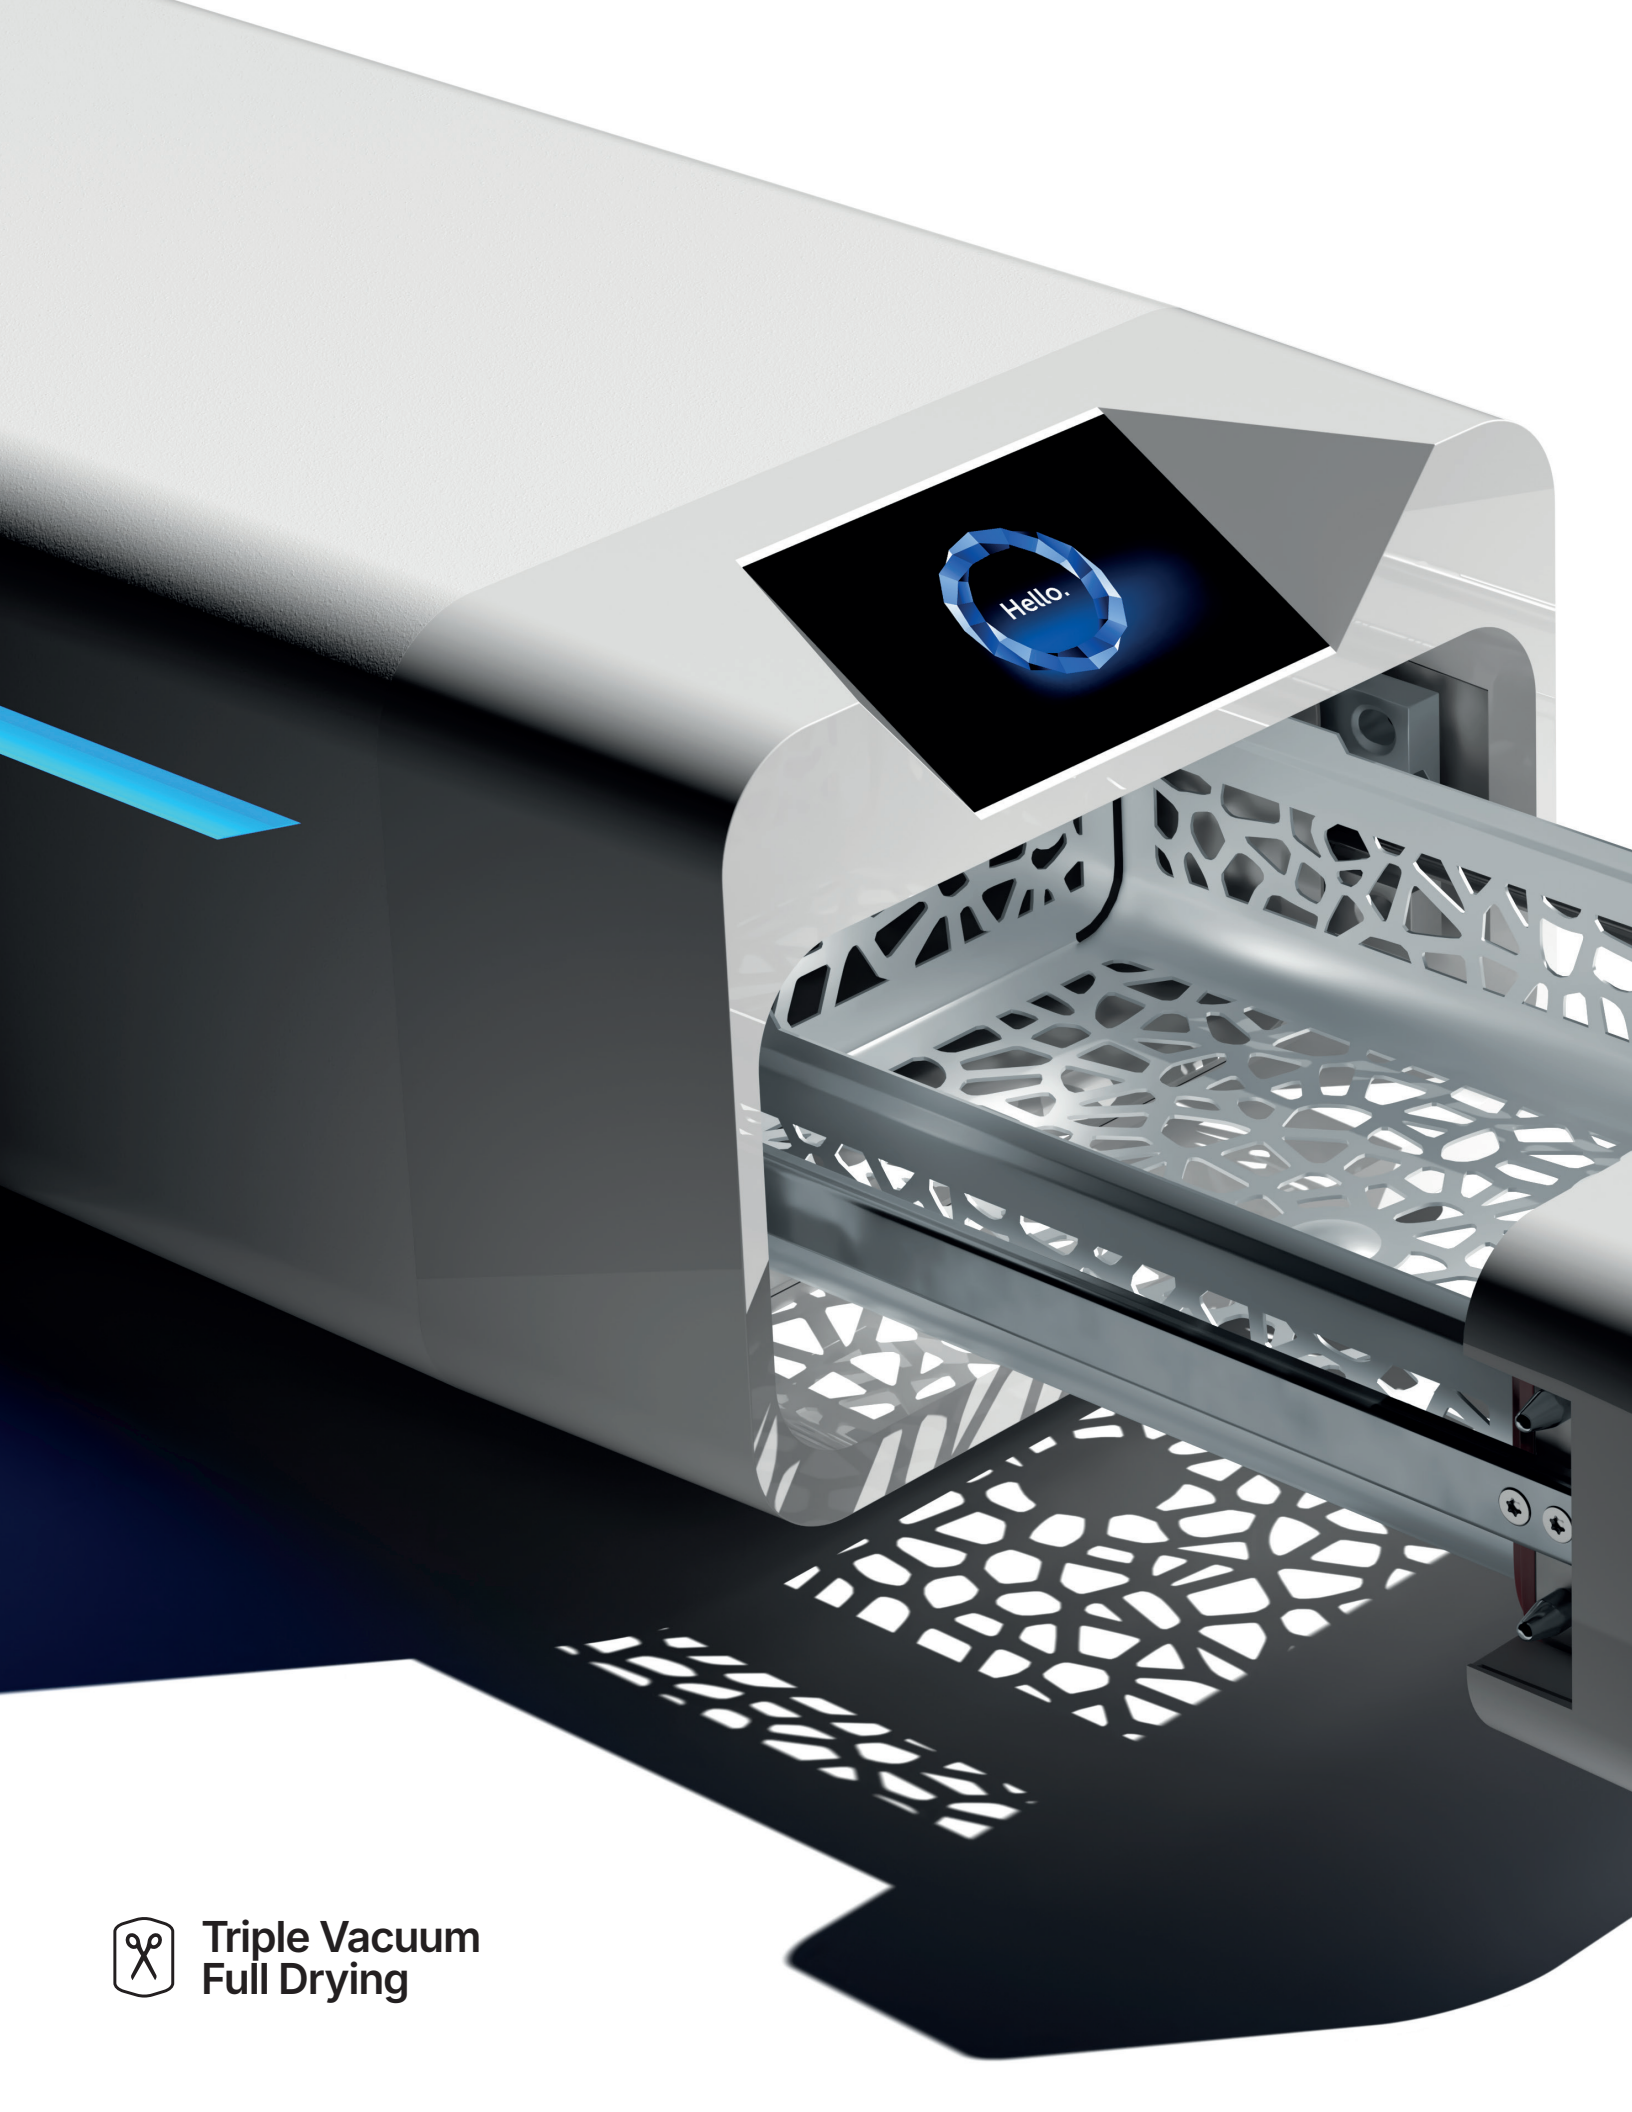


Triple Vacuum
Full Drying

# Enbio PRO

| S / 273°F | B / 273°F | B / 250°F |
|---|---|---|
| **9 min** | **15 min** | **45 min** |
| Unwrapped | Wrapped (pouches) | Delicate instruments |

**16** diagnostic sets OR
**16** handpieces OR
**1 – 4** surgical casettes OR
**1** implant cassette



# Enbio PRO.
# Small footprint. Big space.

Workhorse in a small practice.
Double capacity and space
for implant and surgical cassettes.

**Usable load space**
**11.2 × 7.5 × 2.8 in**

**16** diagnostic sets OR
**16** handpieces OR
**1** surgical casette OR
**1** implant casette

small instrument tray
pouch rack






# Enbio S.
# Speedmaster.

Unbeatable speed in the class.
15 minute vacuum cycle.
Bone dry pouches.

**Usable load space**
**11.2 × 7.1 × 1.3 in**

8 diagnostic sets OR
8 handpieces




# Performance technology inside.




### Die-cast Aluminum Chamber

Patented aluminum alloy chamber is manufactured through an advanced die-casting process that yields exceptional structural integrity and thermal conductivity, ensuring uncompromised performance throughout the device's operational lifespan.

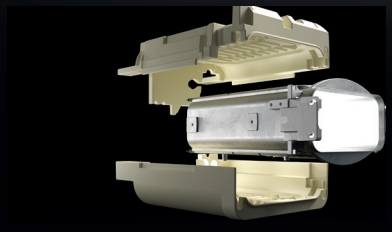

**Polyurethane foam chamber Insulation**

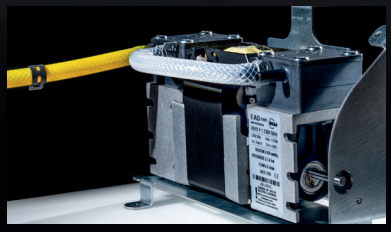

Heavy-duty vacuum pump



## Lifetime warranty


The chamber is covered by a lifetime warranty.

## Structure-integrated heaters

Heating elements are directly integrated into the die-cast chamber structure during production. Seamless thermal interface significantly reduces warm-up intervals while ensuring optimal temperature uniformity.





Fully automatic with touch screen control

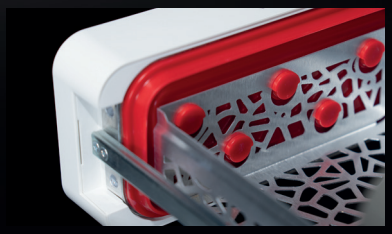

Red sillicone chamber seal with snap-off tray mount

# Enbio PRO

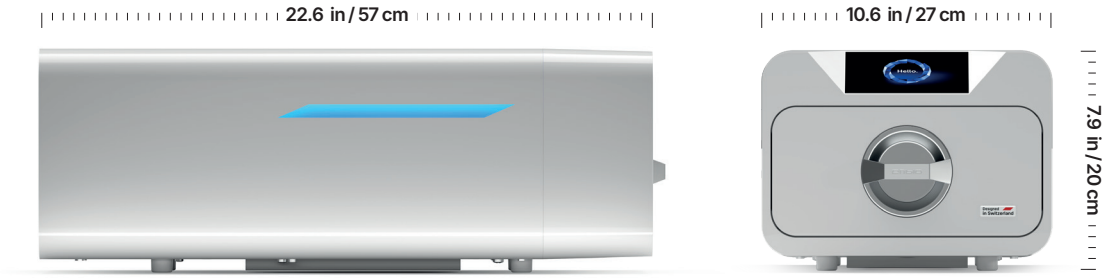







**Usable load space**
## 11.2 × 7.5 × 2.8 in

**Unit weight**
## 44 lbs / 20 kg

**Capacity**

| | |
|---|---|
| Max. packages amount (circa) | **16** |
| Max. recommended batch weight | **1.0 kg / 2.2 lbs** |
| Process chamber volume | **5.3 l** |

**Pressure & temperature**

| | |
|---|---|
| Working pressure | **2.1 Bar / 30.47 psi** |
| Max. pressure | **2.3 Bar / 33.38 psi** |
| Max. process tempreature | **137°C / 278.6°F** |

**Electrical**

| | |
|---|---|
| Power supply | **110-120V AC/60 Hz** |
| Power | **2.45 kW** |
| Max. power consumption | **15 A** |

**Misc**

| | |
|---|---|
| Ingress protection | **IP20** |
| Data archiving | **USB stick** |
| Water conductivity* | **< 15 µS/cm** |

Medical device class II b
EN-13060
93/42/EEC Directive

FDA* Cleared

TÜV NORD

CLEANING STERILIZATION

MDSAP
Medical Device
Single Audit Program

**Enbio Corp.**
**1075 HWY 124,Hoschton G.A. 30548, Bldg 300 Ste 300**

**enbio.com**